

THE REAL DIFFERENCE IN **NERIUMAD'S** CLINICAL TRIALS

The results from NeriumAD's clinical trial are based on hard data output from ST&T's facial scanning equipment, which measures the actual change in the skin. However, many well-known skincare companies base the results from their clinical studies on participants' opinions or the visual grading of doctors, rather than the scientific facial scanning method we employ. This means the efficacy of their products are determined by what subjects think or what a doctor observes, instead of what a computer dictates.


Although NeriumAD's results can easily be seen by the naked eye, the percentages from our clinical trials are based solely on unbiased scientific data.



30-DAY PIGMENT SPOT RESULTS

Facial Analysis Image and Data Comparison


CAKI-508

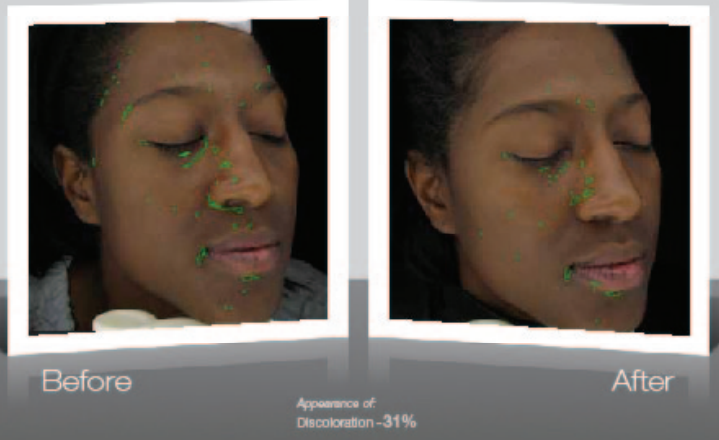

30-DAY WRINKLE RESULTS

Facial Analysis Image and Data Comparison

JEPA-511

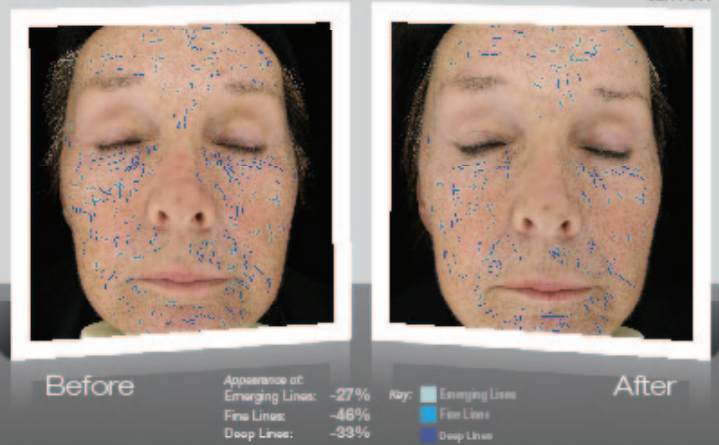

Using the most advanced facial scanning equipment available, ST&T Research set out to thoroughly test the effects of NeriumAD Age-Defying Treatment. ST&T's technology, which includes fluorescence spectroscopy and artificial intelligence, allows them to see what is happening on the skin's surface, as well as what is developing beneath the skin.